



Lambda Transmitter LT3-Ex Combination probe KS1D-Ex

Tel.: (21) 3445.8120

E-mail: engezer@engezer.com.br

Site: www.engezer.com.br

(21) 97144.1593 

@engezer 

Engezer Spengezer 

sergio.engezer 

Engezer Solução em Análise de Gases 



System overview

Lambda transmitter LT3-Ex Combination probe KS1D-Ex

LAMTEC Measuring System LT3-Ex KS1D-Ex.

With the LT3-Ex lambda transmitter, LAMTEC provides customers with a simple device for the simultaneous measurement of oxygen (O_2) and oxidising gas components (CO_e) in an explosion-protected (Ex) design.

Together with the KS1D-Ex combination probe, the lambda transmitter is a system for the measurement of oxygen (O_2) and the detection of oxidising gas components (CO/H_2 , etc.). The probe is installed directly into the process and does not require a gas treatment unit. Both the transmitter and the probe are designed in "flameproof enclosure" (Ex d) type of explosion protection. This makes it possible to use the entire system in explosive atmospheres, both in Zone 1 and Zone 2. Due to the design of the probe and the materials used, such as ceramics and stainless steel, it is very robust and can be used for all kinds of measuring tasks.

Due to the magnetic keyboard, the device can be operated through the closed disc using a magnetic pin. Explosion protection (Ex) is thus always guaranteed, even during maintenance.

Through the use of an exhaust gas deflection tube made of Kanthal, it is possible to use the KS1D probe up to exhaust gas temperatures of 1,200°C.



Operation using magnetic pin.

Advantages:

- O_2 measurement range: 0 - 18 vol. % with limitation 0 - 25 vol. %
- CO_e measurement range: 0 - 1,000 ppm
- Use in explosive atmospheres, approval according to ATEX and IEC
- Handling during operation when the housing is closed
- Not affected by false air (CO_e)
- No gas preparation required, measurement directly in the moist flue gas
- Adjustment time to 60 % value (T_{60}):
 O_2 approx. 50 s CO_e approx. 40 s
- Low heating power with LT3-Ex
15 - 23 W depending on the exhaust gas temperature
- Low-maintenance

Measurement principle

Measurement principle for KS1D-Ex:

The basis of the KS1D-Ex combination probe is a heated electrochemical measuring cell made of zirconium dioxide ceramics.

It has 3 electrodes:

- O_2 -sensitive platinum electrode
- CO/H_2 -sensitive electrode made from a platinum/gold alloy
- Platinum reference electrode

The O_2 measuring cell works as an electrochemical concentration chain and generates a direct voltage. Supplying the external electrode with a sample gas and the internal electrode with a reference gas of a familiar O_2 concentration, e.g., air (20.96 % O_2), with a continuous constant temperature between 700 and 800°C, results in the logarithmic association between the probe voltage U and the oxygen concentration on the sample gas.

Probe principle - CO/H_2 -sensitive electrode:

Alongside Nernst voltage U_{O_2} which is determined by the oxygen content, the combustible components in the sample gas generate an auxiliary direct voltage U_{CO/H_2} . The sensor voltage is the sum of both voltages $U_S = U_{O_2} + U_{CO/H_2}$ (see "Sensor characteristic curve"). As already in the case of low concentrations of oxidising gases, such as H_2 or CO , the mixed potential is considerably higher than the O_2 signal.


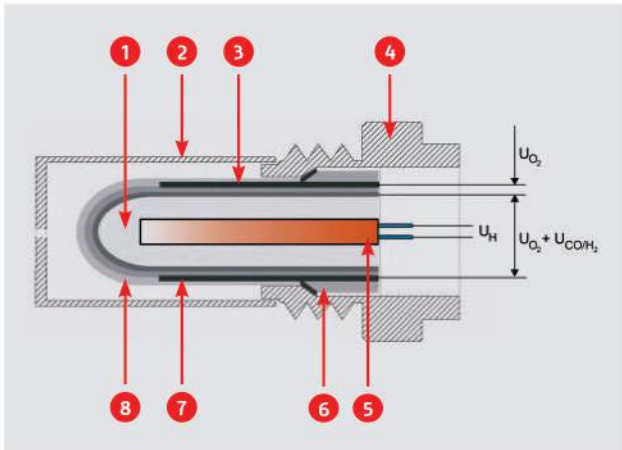


Diagram of the combination probe KS1D-Ex.

- | | |
|---------------------------------------|---|
| 1 Reference electrode | 2 Sensor cap with gas inlet |
| 3 O ₂ -sensitive electrode | 4 Housing |
| 6 Functional ceramics | 7 CO/H ₂ sensitive electrode |
| 8 Protective coating | |

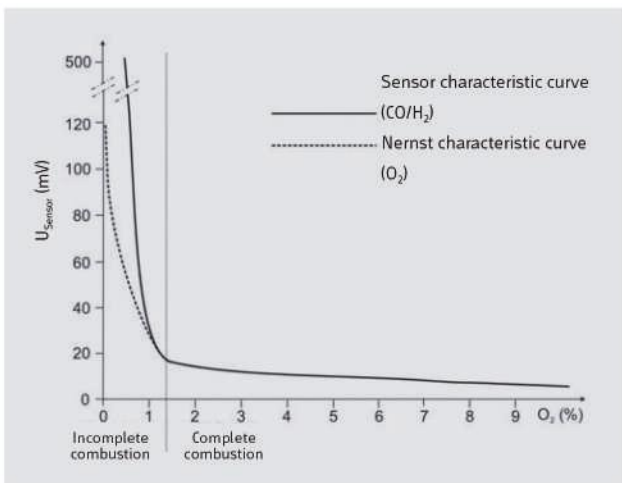

Sensor characteristic curve.

The principle of oxygen measurement is really simple and was already described by W. H. Nernst at the end of the nineteenth century. The voltage U between the two electrodes is composed of a constant offset voltage U_0 and a variable voltage, which, on the one hand, depends on the sensor temperature and, on the other hand, on the ratio of oxygen content to the reference and measurement side:

$$U = U_0 + k \cdot T \cdot \ln(p_{O_2, \text{meas}} / p_{O_2, \text{ref}})$$

k is a natural constant. This formula (Nernst formula) explains that the larger the difference between the oxygen fractions in the sample gas and in the reference gas, the greater the sensor voltage is. The offset voltage generally arises as a result of temperature differences between the reference electrode and the electrode in the sample gas.

On both electrodes, the conversion of oxygen to ions takes place ($O_2 + 4e \rightarrow 2O^{2-}$). The back reaction takes place to the same degree in the chemical balance. The differ-

ence in the concentration of oxygen on both sides, however, results in more oxygen being converted than on the sample side when all the framework conditions are met on the reference side. This results in different potentials on both sides. The potential difference produces the measured voltage depending on the oxygen fraction in the sample gas (the reference side is always constant).

Functional principle CO_e measurement:

If the sample gas does not comprise pure air or nitrogen and oxygen, but also contains a fraction of combustible gases (CO, H₂, CH₄, etc. → CO_e), several effects are responsible for the occurrence of the measured voltage.

The first voltage fraction is the same as in oxygen measurement. The difference between the oxygen fractions also exists in this case. The second voltage fraction is the so-called CO_e voltage. This is added together with the voltage from the oxygen difference to the overall voltage measured between the electrodes U_{CO/H_2} .

$$U_{CO/H_2} = U_{O_2} + U_{CO_e}$$

The mechanisms which contribute to the formation of the U_{CO_e} voltage are far more complex than the operation of oxygen measurement. Therefore only the most important points should be mentioned here in brief.

- The sensor. To measure CO_e, it is necessary to alter the material of the sensing electrode as a pure platinum electrode does not respond to CO_e as desired. As a rule, in CO_e sensors the sensing electrode is "contaminated" with other metals.
- Platinum has the property of binding many gases including O₂ and CO_e to the surface in an active state. The CO_e bound to the surface reacts spontaneously with the bound oxygen as platinum is a very good catalyst.
- Gold does not have this property of platinum described. However, it binds CO_e molecules to its surface very well. Oxygen, which was there previously, is therefore displaced. In the end, this results in no more oxygen being present anywhere where there is gold on the surface. Therefore the desired balance of the oxygen fractions between both electrodes (see oxygen measurement) is shifted further towards an imbalance.

The catalytic reactions, the oxygen imbalance and additional processes not described here altogether form the sensor voltage which is determined when measuring CO_e. If the known fraction of oxygen is deducted from this total voltage, the pure voltage which arises as a result of the CO_e processes is obtained.

Exhaust gas deflection tube

The exhaust gas deflection tube was developed to cool off hot combustion system flue gases and to control the probe. The hot flue gas is trapped in the flue gas duct and conducted to the probe through the bottom part of the deflection tube. In the process, the flue gas cools off. After the probe, the cooled flue gas is conducted back to the flue gas duct through the top part of the deflection tube.

1 Combination probe KS1D-Ex **2** Exhaust gas deflection tube length **3** Counterflange DN65 PN6 **4** Flange seal **5** Graphite seal


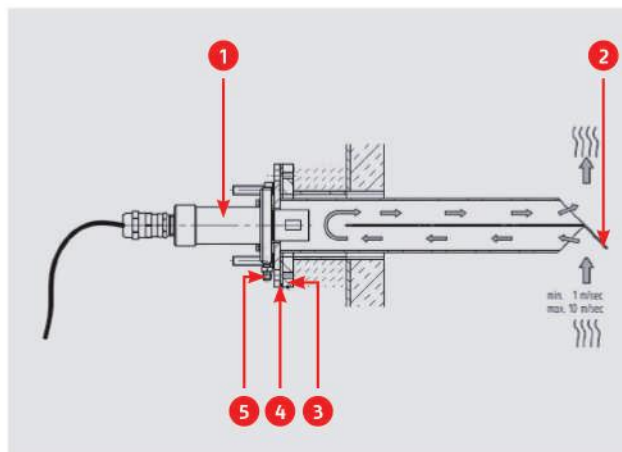


Diagram of the combination probe KS1D-Ex.



Overview of functions for LT3-Ex with KS1D-Ex.

Basic system.

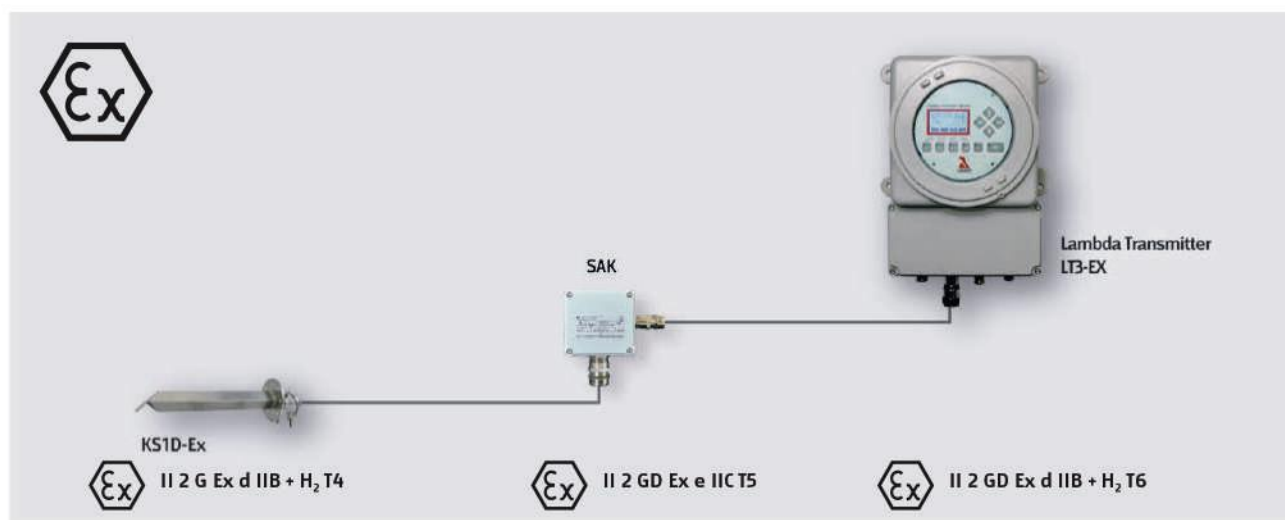

Lambda transmitter LT3-Ex with SAK and main switch.

The LT3-Ex lambda transmitter is a microprocessor-based measuring transducer with diagnosis function.

Specification:



CE 0081 Ex II 2 GD
Ex d IIB+H2 T6
Ex tD A21 IP65 T85°C
LCIE 08 ATEX 6038X

The device is operated using a magnetic pin with the housing closed so that no special measures are required during operation in explosive atmospheres.



Combination probe KS1D-Ex.

Combination probe KS1D-Ex

Specification:



II2G Ex d IIB+H2 T4 (Ta: -20°C to 60°C.
LCIE 13 ATEX 3045X IECEx
LCIE 13.0027X

For the first time, the combination probe KS1D-Ex enables the simultaneous measurement of oxygen (O₂) and oxidising exhaust gas components (CO/H₂) using a ZrO₂ sensor. For the KS1D-Ex, the measuring principles of the proven lambda probe LS2 and combination probe KS1 is combined in a ZrO₂ sensor.

The probe is designed in a flameproof enclosure and can be used in Zone 1 and Zone 2 explosive atmospheres.

Optional components.

PCB probe connection box

The LAMTEC PCB probe connection box has been designed to bridge longer distances between the LT3 and the probe without need for an extension cable (> 2 metres). Here, on the LT3-Ex, the probe connection jack and the blank cover replace the standard screwed cable gland. The PCB contains a terminal strip and the conversion for the probe connector.



Notes.

Notes.

**Caso queira adaptar este produto a suas necessidades
usando um sistema de condicionamento, uma
automação ou formando um produto, contate:**

COMERCIAL@ENGEZER.COM.BR

**para mais informações ou preços*



ENGEZER

SOLUÇÕES EM ANÁLISE DE
GASES



(21) 97144.1593



@engezer



Engezer
Spengezer



sergio.engezer



Engezer Solução
em Análise de
Gases

Tel.: (21) 3445.8120 : **E-mail:** engezer@engezer.com.br : **Site:** www.engezer.com.br